



Drug-device combination products

MDR Article 117:

Drug-device combination products application process

Introduced by the European Commission under the Medical Devices Regulation (MDR), Article 117 requires manufacturers placing drug-device combination products onto the market as an integral device and marketing them as a “medicinal product” to seek a Notified Body Opinion (NBOp). The notified body then confirms whether the device is compliant with the relevant General Safety and Performance Requirements (GSPR) and provides an NBOp Report to the manufacturer to include in the Market Authorisation Application (MAA).

What is the role of a notified body?

A notified body, such as BSI, is designated by the Competent Authority to conduct a conformity assessment under the relevant EU regulations. For specific drug-device combination products, the conformity assessment requires a review of the relevant Technical Documentation provided by the manufacturer in support of the safety and performance claims for their medical device. The Technical Documentation is assessed against the GSPR of the EU regulations, taking into consideration the relevant guidance set out by the EU.

Focusing our attention on Article 117

BSI has formed a dedicated *Medicinal and Biologics* team to provide guidance on Article 117. The team has over 55 years' combined experience in drug development, Good Manufacturing Procedures (GMP) systems and controls, and Quality by Design (QBD). The team also has extensive experience in conformity assessments of medical devices with ancillary medicinal substances (MDR Rule 14) and substance-based medical devices (MDR Rule 21).

BSI was the first in the world to issue an NBOp to a manufacturer under Article 117 of the MDR. This is thanks to the incredible hard work of the team to provide this expertise to clients.

“The formation of a new, dedicated team will allow us to focus our attention on this challenging area of new EU regulation, delivering excellence to our clients.”

Dr Jennifer Durrant

Global Head of Medicinal and Biologics, BSI

Examples of drug-device combination products requiring Notified Body Opinion



Drug-device combinations

Autoinjector

Inhaler

Pre-filled nebuliser

Pre-filled pen

Pre-filled syringe

Transdermal patch

FAQs about the Article 117 process

Q: How long does the Article 117 process take?

The duration of the entire process depends on the quality of the documentation submitted by the manufacturer, the number of questions BSI needs to ask for each round, and the manufacturer's responsiveness in answering questions. We have included an estimated timeline for Article 117 reviews on the next page. The process is typically expected to take between two and six months to complete, so the more time you factor into the process, the better.

Q: Is there an expedited service available?

There is no expedited service; however, our team will work closely with you to complete the reviews within the estimated timelines on the next page.

Q: Which documents do I need to supply?

Annex II of the MDR provides guidance on which documents are required. BSI has also produced an [MDR Documentation Submission Best Practice Guidelines](#) for further guidance. As part of the Article 117 process, there will be a thorough review of evidence of conformity to the GSPP; for this reason, supporting technical data will be required.

Q: What is the output of the process?

BSI will issue an NBOp Report providing a recommendation on conformity of the drug-device combination product to Article 117 of the MDR. To avoid any duplication of the reviews, this report will be detailed enough to demonstrate to the Competent Authority what data have been reviewed and to assure them conformity has been appropriately assessed.

Q: What is the role of BSI during the question stage of the MAA process?

On rare occasions, there might be questions from the Competent Authorities for the Notified Body during the MAA process. BSI will be available to answer these, mindful of the fact that there is a clock stop.


Q: How much clinical data is required?

The safety and efficacy of the medicinal substance is reviewed by the Competent Authority. As a Notified Body, BSI will need sufficient data to demonstrate the device performs as intended in the clinical setting. Clinical data may be required if there are specific device-related clinical claims or safety concerns.

Q: I'm making a change to an already marketed drug-device combination product. Does this require an NBOp?

Substantial changes to your product that could affect the performance and safety characteristics of the medical device will require an NBOp as part of the variation process. As an independent Notified Body, BSI is not able to advise or provide consultation to manufacturers on whether specific changes require an NBOp.

Estimated timeline for Article 117 reviews

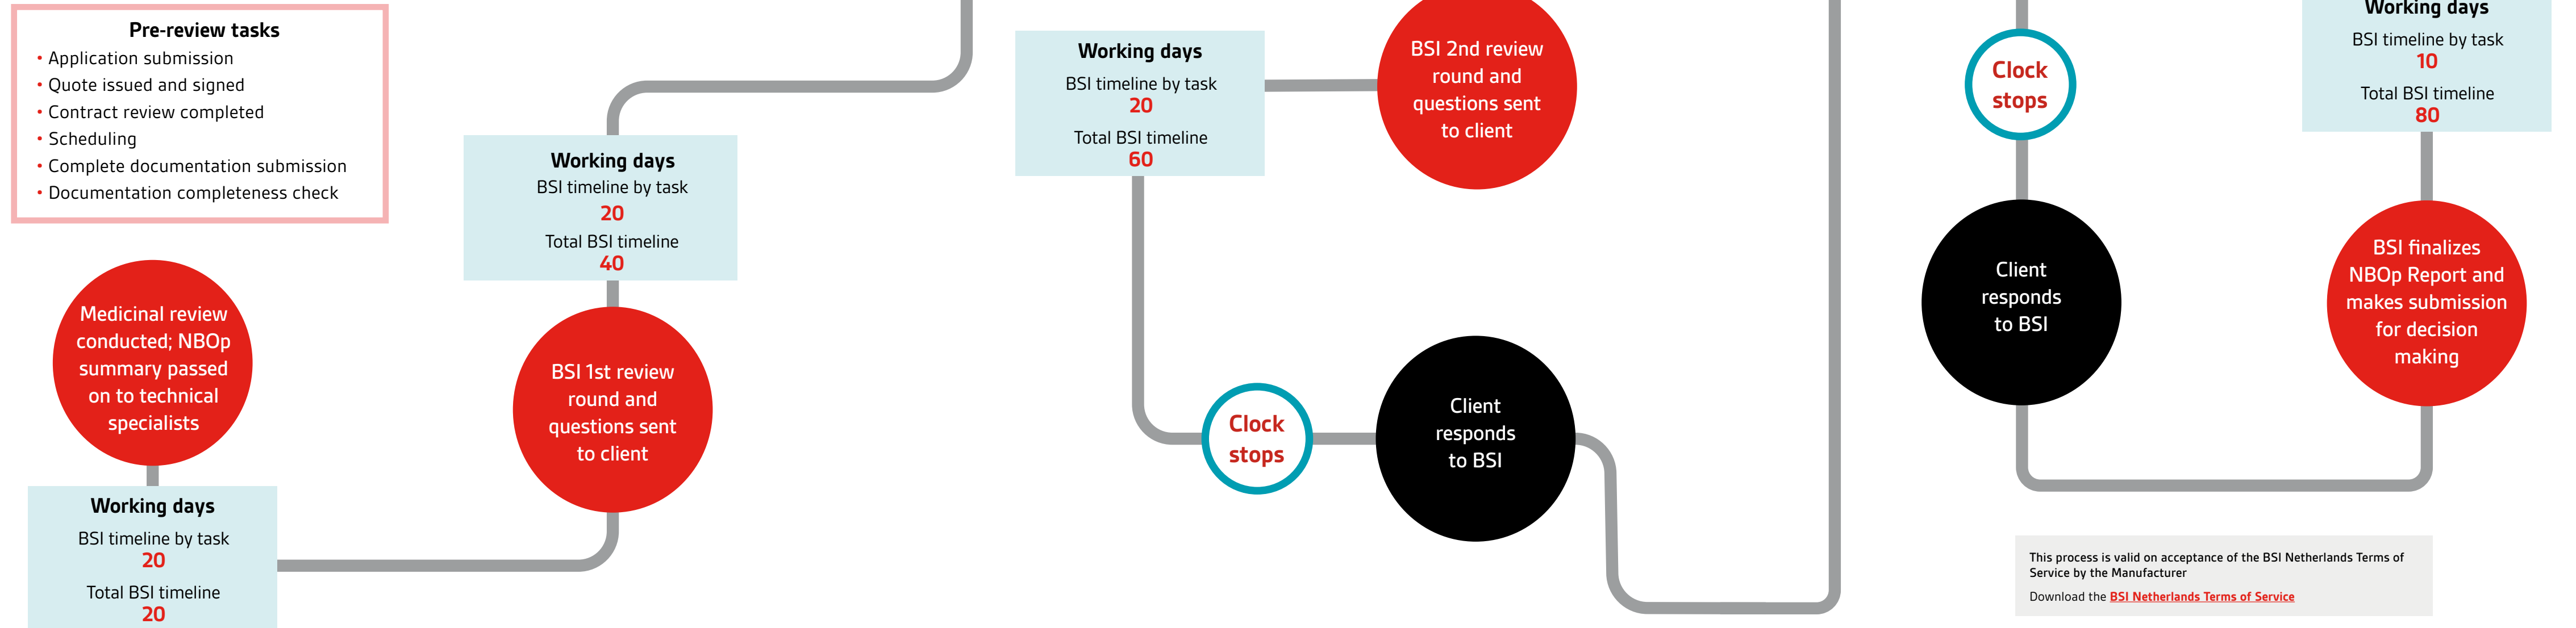

Your resource for excellence

Talk to BSI

- We have 4,600 colleagues globally
- 84 offices in 31 countries across the world
- Over 84,000 clients operating in 195 countries across a range of industries
- Together, our clients account for 83% of the FTSE 100, 53% of the Fortune 500, and 81% of the Nikkei 225
- Over 750 colleagues within BSI Medical Devices

Additional services

Medical device newsletter service

Keep updated on what's happening in the industry and changes in regulatory and quality requirements. You can take advantage of this free service by signing up on our website: bsigroup.com/medical

Informative webinars

Hear regular updates from our experts on key topics; listen live or listen back.

Comprehensive whitepapers

Our technical specialists collaborate with external experts to bring you the latest views and understanding on complex regulatory issues. Download your complimentary copies from our website: bsigroup.com/medical

Medical device guidance documents

Our online guidance documents provide assistance in understanding the regulatory requirements for medical devices.

Standards

BSI British Standards delivers leading best practice solutions through the development and publication of more than 59,000 standards and related products.

Your resource in worldwide compliance: call BSI today on **+91 400 86 20**
or visit bsigroup.com/medical – to start your journey.

BSI UK Approved Body (0086)

Kitemark Court
Davy Avenue, Knowlhill
Milton Keynes MK5 8PP
United Kingdom
T: +44 345 080 9000
T: +44 1908 814920
E: eu.medicaldevices@bsigroup.com

BSI Group America Inc.

12950 Worldgate Drive
Suite 800
Herndon, VA 20170
USA
T: +1 800 862 4977/703 437 9000
F: +1 703 437 9001
E: us.medicaldevices@bsigroup.com

BSI Notified Body (2797)

Say Building
John M. Keynesplein 9
1066 EP Amsterdam
The Netherlands
T: +31 20 346 0780
F: +31 20 346 0781
E: eu.medicaldevices@bsigroup.com

BSI Group Asia Pac

BSI Group – Hong Kong
23rd Floor, Cambridge House
TaiKoo Place, 979 King's Road
Island East Hong Kong
T: +852 3149 3320

BSI Group Iberia SAU

C/ Juan Esplandiú 15 - 3ª planta
28007, Madrid
T: +34 91 400 86 20
E: info.esp@bsigroup.com



...making excellence a habit.™